

Люкметры портативные DELTA ОНМ HD2102.1, HD2102.2

Технические характеристики

Архангельск (8182)63-90-72
Астана (7172)727-132
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89
Иваново (4932)77-34-06

Ижевск (3412)26-03-58
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Липецк (4742)52-20-81
Киргизия (996)312-96-26-47

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Казахстан (772)734-952-31

Пермь (342)205-81-47
Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Таджикистан (992)427-82-92-69

Сургут (3462)77-98-35
Тверь (4822)63-31-35
Томск (3822)98-41-53
Тула (4872)74-02-29
Тюмень (3452)66-21-18
Ульяновск (8422)24-23-59
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Ярославль (4852)69-52-93

Единый адрес для всех регионов: dmh@nt-rt.ru || www.deltaohm.nt-rt.ru

HD2102.1 - HD2102.2



HD2102.1, HD2102.2 PHOTO-RADIOMETERS

HD2102.1 and HD2102.2 are portable instruments with LCD display. They measure illuminance, luminance, par and irradiance (across VIS-NIR, UVA, UVB and UVC spectral regions or measurement of irradiance effective according to the UV action curve).

The probes are equipped with the SICRAM automatic detection module: in addition to detection, the unit of measurement selection is also automatic. The factory calibration data are already stored inside probes.

In addition to instantaneous measurement the instruments calculate the acquired measurements time integral Q(t). Some thresholds can be associated with the integrated measurement and with the integration time, which can be set in the menu. When exceeded, these thresholds cause the instrument to stop the integral calculation.

The HD2102.2 instrument is a **datalogger**. It memorizes up to 38,000 samples with single probes and 14,000 with combined probes. Data can be transferred from the instrument connected to a PC via the RS232C serial port or USB 2.0 port. The storing interval, printing, and baud rate can be configured using the menu.


Both models are fitted with an RS232C serial port and can transfer the acquired measurements in real time to a PC or to a portable printer.

The **Max**, **Min** and **Avg** function calculate the maximum, minimum or average values.

Other functions include: the relative measurement REL, the HOLD function, and the automatic turning off that can also be disabled.

The instruments have IP66 protection degree.

INSTRUMENT TECHNICAL CHARACTERISTICS	
Measured quantities	lux - fcd - lux/s - fcd/s - W/m ² - μW/cm ² J/m ² - μJ/cm ² - μmol/(m ² s) - μmol/m ² - cd/m ² - μW/lumen
Power Supply	
Batteries	4 1.5V type AA batteries
Autonomy	200 hours with 1800 mAh alkaline batteries
Power absorbed with instrument off	20 μA
Mains (SWD10)	Output mains adapter 12 Vdc / 1A
Security of memorized data	Unlimited, independent of battery charge conditions
Measured values storage - model HD2102.2	
Type (for single probes)	2000 pages containing 19 samples each
Type (for combined probes)	2000 pages containing 7 samples each
Quantity (for single probes)	total of 38000 samples
Quantity (for combined probes)	total of 14000 samples
Selectable storage interval	1, 5, 10, 15, 30 s 1, 2, 5, 10, 15, 20, 30 min 1 hour
Serial interface RS232C	
Type	RS232C electrically isolated
Baud rate	can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Print interval	immediate or selectable between: 1, 5, 10, 15, 30 s 1, 2, 5, 10, 15, 20, 30 min 1 hour
USB interface - model HD2102.2	
Type	1.1 - 2.0 electrically isolated
Connections	
Input module for the probes	8-pole male DIN45326 connector
RS232 serial interface	8-pole MiniDin connector
USB serial interface	B-type MiniUSB connector
Mains adapter	2-pole connector (positive at centre)
Time	
Date and time	in real time
Accuracy	1min/month max drift
Operating conditions	
Working temperature	-5...50 °C
Storage temperature	-25...65 °C
Working relative humidity	0...90% RH without condensation
Protection degree	IP66
Instrument	
Dimensions (Length x Width x Height)	185 x 90 x 40 mm
Weight	470 g (complete with batteries)
Material	ABS, rubber
Display	2x4½ digits plus symbols Visible area: 52x42 mm

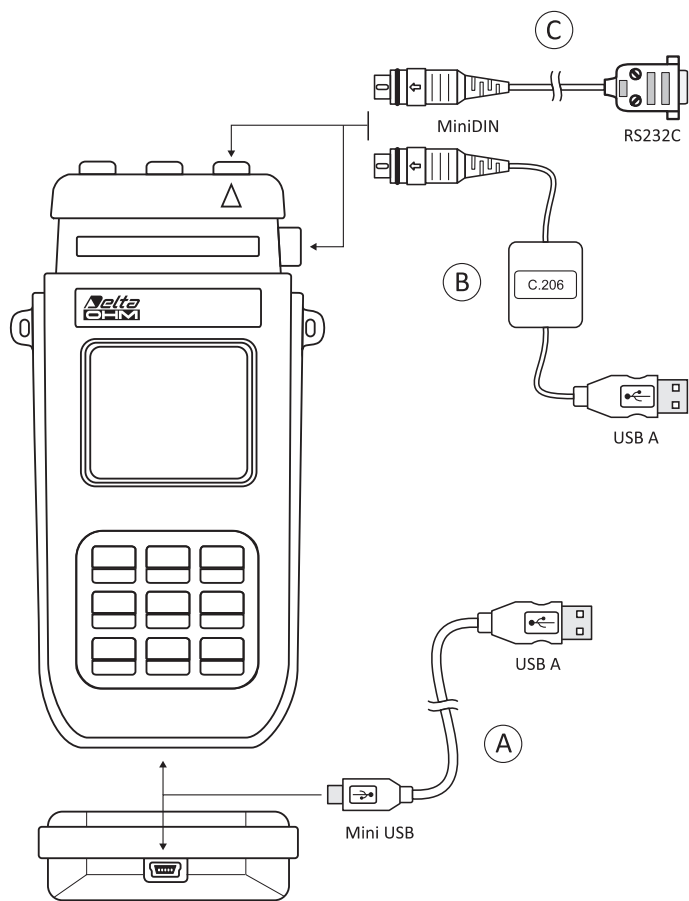

A In the **HD2102.2** models of portable data logger, a new serial port miniUSB type HID (Human Interface Device) has been implemented. When making the connection to the PC by the USB cable Type A - Mini USB B-type coded CP23, no USB driver installation is requested.

B For the connection of the models **HD2102.1** to the RS232 port of your PC, the USB/serial converter is available (code **C.206**). The converter is equipped with its own drivers that have to be installed before connecting the converter to the PC.

C The port with the MiniDIN connector which is present on every model is an RS232C type. By means of the cable coded HD2110CSNM, an RS232C port of a PC or the HD40.1. printer can be connected.



HD2110CSNM



CP23



ORDERING CODES

HD2102.1: The kit is composed by the instrument HD2102.1, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software downloadable from Delta OHM website.

HD2102.2: The kit is composed by the instrument HD2102.2 **data logger**, 4 1.5V alkaline batteries, USB cable CP23, operating manual, case and DeltaLog9 software downloadable from Delta OHM website

Probes and cables have to be ordered separately.

Accessories

HD2110CSNM: 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

C.206: Cable for instruments of the series HD21...1 for direct connection to the USB input of a PC.

SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.

HD40.1: The kit includes: 24-column portable thermal printer, serial interface RS232, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. It uses the optional cable HD2110 CSNM.

Probes with SICRAM module - for technical specifications of the probes, see following pages.

LP471PHOT: Photometric probe for ILLUMINANCE measurement.

LP471LUM2: Photometric probe for LUMINANCE measurement.

LP471PAR: Quantum radiometric probe for the measurement of the PHOTONS FLOW across the chlorophyll range PAR (Photosynthetically Active Radiation 400 nm...700 nm).

LP471PAR02: Quantum-radiometric probe for measuring the PHOTONS FLOW in the chlorophyll field PAR (photosynthetically Active Radiation 400 nm...700 nm). Special filter that optimizes the spectral response.

LP471RAD: Radiometric probe for IRRADIANCE measurement in the 400 nm...1050 nm spectral range.

LP471UVA: Radiometric probe for measuring the IRRADIANCE in the UVA spectral range 315 nm...400 nm.

LP471UVB: Radiometric probe for measuring the IRRADIANCE in the UVB spectral range 280 nm...315 nm.

LP471UVC: Radiometric probe for measuring the IRRADIANCE in the UVC spectral range 220 nm...280 nm.

LP471UVBC: Radiometric probe for measuring the IRRADIANCE in the UV-BC spectral range 210 nm...355 nm.

LP471BLUE: Radiometric probe for EFFECTIVE IRRADIANCE measurement in the spectral range of Blue light.

LP471P-A: Combined probe for measuring the ILLUMINANCE (lux), with standard photopic spectral response, and for measuring the IRRADIANCE (W/m^2) in the UVA spectral range (315...400 nm).

LP471A-UVeff: Combined probe for measuring the TOTAL EFFECTIVE IRRADIANCE (W/m^2) weighted according to the UV action curve.

LP471SILICON-PYRA: Pyranometer with silicon photodiode to measure the GLOBAL SOLAR IRRADIANCE, diffuser for cosine correction. Spectral range: 400...1100 nm.

LP471PYRA03.5: Probe consisting of Spectrally Flat Class C (Second Class) pyranometer LPPYRA03 and a 5 m long cable complete with SICRAM module.

LP471PYRA02.5: Probe consisting of Spectrally Flat Class B (First Class) pyranometer LPPYRA02 and a 5 m long cable complete with SICRAM module.

LP471PYRA10.5: Probe consisting of Spectrally Flat Class A (Secondary Standard) pyranometer LPPYRA03 and a 5 m long cable complete with SICRAM module.








LPBL: Base with levelling device (not suitable for LP471LUM2 and LP471PYRA... probes).

LPBL3: Adjustable wall support for \varnothing 30 mm photometric and radiometric probes.

RADIOMETRIC-PHOTOMETRIC PROBES FOR PORTABLE INSTRUMENTS

Code	Description	
LP471PHOT	Photometric probe for measuring ILLUMINANCE , spectral response according to the photopic curve, class B according to CIE N° 69, cosine correction diffuser. Measuring range: 0.1 lux...200·10 ³ lux.	
LP471LUM2	Photometric probe for measuring LUMINANCE , spectral response according to the photopic curve, angular field 2°. Measuring range: 1 cd/m ² ...2000·10 ³ cd/m ² .	
LP471PAR	Quantum-radiometric probe for measuring PHOTONS FLOW in the chlorophyll field PAR (photosynthetically Active Radiation 400 nm...700 nm), μmol m ⁻² s ⁻¹ measure, cosine correction diffuser. Measuring range: 0.1 μmol m ⁻² s ⁻¹ ...10·10 ³ μmol m ⁻² s ⁻¹	
LP471PAR02	Quantum-radiometric probe for measuring the PHOTONS FLOW in the chlorophyll field PAR (photosynthetically Active Radiation 400 nm...700 nm), μmol m ⁻² s ⁻¹ measure, opaline quartz diffuser for cosine correction. The probe uses a special filter that optimizes the spectral response. Measuring range: 0.1 μmol m ⁻² s ⁻¹ ...10·10 ³ μmol m ⁻² s ⁻¹ .	
LP471RAD	Radiometric probe for measuring IRRADIANCE in the spectral range 400 nm...1050 nm, cosine correction diffuser. Measuring range: 1.0·10 ⁻³ W/m ² ...2000 W/m ² .	
LP471UVA	Radiometric probe for measuring IRRADIANCE in the UVA spectral range 315 nm...400 nm, peak at 360 nm, quartz diffuser for cosine correction. Measuring range: 1.0·10 ⁻³ W/m ² ...2000 W/m ² .	
LP471UVB	Radiometric probe for measuring IRRADIANCE in the UVB spectral range 280 nm...315 nm, peak at 305 nm...310 nm, quartz diffuser for cosine correction. Measuring range: 1.0·10 ⁻³ W/m ² ...2000 W/m ² .	
LP471UVC	Radiometric probe for measuring IRRADIANCE in the UVC spectral range 220 nm...280 nm, peak at 260 nm, quartz diffuser for cosine correction. Measuring range: 1.0·10 ⁻³ W/m ² ...2000 W/m ² .	
LP471UVBC	Radiometric probe for measuring the IRRADIANCE in the UV-BC spectral range 210 nm...355 nm, peak at 265 nm, quartz diffuser for cosine correction. Measuring range: 1.0·10 ⁻³ W/m ² ...2000 W/m ² .	

RADIOMETRIC-PHOTOMETRIC PROBES FOR PORTABLE INSTRUMENTS

Code	Description	
LP471BLUE	Radiometric probe for measuring the EFFECTIVE IRRADIANCE in the spectral range of the BLUE LIGHT 380 nm...550 nm, diffuser for cosine correction. Measuring range: $1.0 \cdot 10^{-3} \text{ W/m}^2 \dots 2000 \text{ W/m}^2$.	 <p>LP 471 Blue Radiance Meter Cosine Cor. Spectral Range: 380 nm...550 nm Peak: 450 nm Measuring range: 2000 W/m²</p>
LP471P-A	Combined probe for measuring ILLUMINANCE (lux), with standard photopic response, and IRRADIANCE ($\mu\text{W/cm}^2$) in the UVA spectral range (315...400 nm, with peak at 360 nm). Both the sensors are equipped with diffuser for the correction according to the cosine law. Illuminance measuring range: $0.3 \text{ lux} \dots 200 \cdot 10^3 \text{ lux}$. Irradiance measuring range: $1.0 \cdot 10^{-3} \text{ W/m}^2 \dots 2000 \text{ W/m}^2$. This probe provides the ratio between UVA irradiance and illuminance in $\mu\text{W/lumen}$ (quantity of interest in museums).	 <p>LP 471 P-A Two channel probe Cosine Corrector Lux Meter - Photopic UVA Irradiance Meter - 2500</p>
LP471A-UVeff	Combined probe for measuring the TOTAL EFFECTIVE IRRADIANCE (W/m^2) weighted according to the UV action curve. The probe is made of two sensors for the correct measure of the Total Effective Irradiance in the range 250...400 nm. Both these sensors are equipped with a diffuser for the correction according to the cosine law. This probe supplies the Total effective irradiance (E_{eff}), the UV-CB effective irradiance and the UVA irradiance. Total effective irradiance measuring range: $0.010 \text{ W/m}^2 \dots 20 \text{ W/m}^2$. B_C effective irradiance measuring range: $0.010 \text{ W/m}^2 \dots 20 \text{ W/m}^2$ UVA irradiance measuring range: $0.1 \text{ W/m}^2 \dots 2000 \text{ W/m}^2$	 <p>LP 471 A-UV eff Two channel probe Cosine Corrector Spectral Irradiance Meter Spectral range: 250...400 nm</p>
LP471 SILICON-PYRA	Pyranometer with silicon photodiode for measuring the GLOBAL SOLAR IRRADIANCE , diffuser for cosine correction. Spectral range 400...1100 nm. Measuring range: $0 \dots 2000 \text{ W/m}^2$. Fixed cable 5 m long with SICRAM module.	 <p>LP 471 Silicon-Pyran 11012114 1024.3 mV/(kW/m²)</p>
LP471PYRA...	The probes LP471PYRA... consist of a pyranometer LPPYRA03, LPPYRA02 or LPPYRA10 and a SICRAM module equipped with a 5 m cable for the connection to the instruments DO9847, HD2102.1, HD2102.2, HD2302.0 and get a reading expressed directly in W/m^2 . LPPYRA03 is a Spectrally Flat Class C (Second Class) pyranometer; LPPYRA02 is a Spectrally Flat Class B (First Class) pyranometer and LPPYRA10 is a Spectrally Flat Class A (Secondary Standard) pyranometer.	
LPBL	Base with levelling device (not suitable for LP471LUM2 and LP471PYRA... probes).	
LPBL3	Adjustable wall support for $\varnothing 30 \text{ mm}$ photometric and radiometric probes.	



LP471PHOT - Probe for the measure of ILLUMINANCE				
Measuring range (lux):	0.10...199.99	...1999.9	...19999	...199.99·10 ³
Resolution (lux):	0.01	0.1	1	0.01·10 ³
Spectral range:	in agreement with standard photopic curve V(λ)			
Class	B			
Calibration uncertainty:	<4%			
f ₁ (in agreement with photopic response V(λ)):	<6%			
f ₂ (response according to the cosine law):	<3%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	<0.5%			
f ₅ (fatigue):	<0.5%			
α (temp. coefficient) f ₆ (T)	<0.05%K			
Drift after 1 year:	<1%			
Working temperature:	0...50°C			
Reference Standards	CIE n.69 - UNI 11142			

Photometric probe for **ILLUMINANCE** measurement, spectral response in agreement with standard photopic vision, diffuser for cosine correction. Measurement range: 0.10 lux...200·10³ lux.




LP471LUM2 - Probe for the measure of LUMINANCE				
Measuring range (cd/m ²):	1.0...1999.9	...19999	...199.99·10 ³	...1999.9·10 ³
Resolution (cd/m ²):	0.1	1	0.01·10 ³	0.1·10 ³
Optical angle:	2°			
Spectral range:	in agreement with standard photopic curve V(λ)			
Class:	C			
Calibration uncertainty:	<5%			
f ₁ (in agreement with photopic response V(λ)):	<8%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	<0.5%			
f ₅ (fatigue):	<0.5%			
α (temp. coefficient) f ₆ (T)	<0.05%K			
Drift after 1 year:	<1%			
Working temperature:	0...50°C			
Reference Standards:	CIE n.69 - UNI 11142			

Photometric probe for **LUMINANCE** measurement, spectral response in agreement with standard photopic vision, vision angle 2°. Measurement range: 1 cd/m²...2000·10³ cd/m².



Typical response curve: LP471PHOT and LP471LUM2

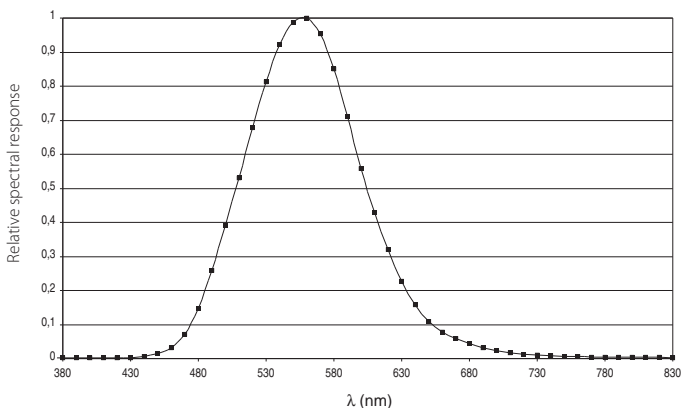


LP471PAR - Quantum radiometric probe for the measure of the PHOTON FLOW across the chlorophyll range PAR			
Measuring range (μmol·m ⁻² ·s ⁻¹):	0.10...199.99	200.0...1999.9	2000...10000
Resolution (μmol·m ⁻² ·s ⁻¹):	0.01	0.1	1
Spectral range:	400 nm...700 nm		
Calibration uncertainty:	<5%		
f ₂ (response according to the cosine law):	<6%		
f ₃ (linearity):	<1%		
f ₄ (instrument reading error):	±1 digit		
f ₅ (fatigue):	<0.5%		
Drift after 1 year:	<1%		
Working temperature:	0...50°C		

Quantum radiometric probe for the measurement of the photonflow across the chlorophyll range **PAR** (Photosynthetically Active Radiation 400 nm...700 nm), measurement in μmol/m²s. Measurement range: 0.10 μmol·m⁻²·s⁻¹...10·10³ μmol·m⁻²·s⁻¹.



Typical response curve: LP471PAR

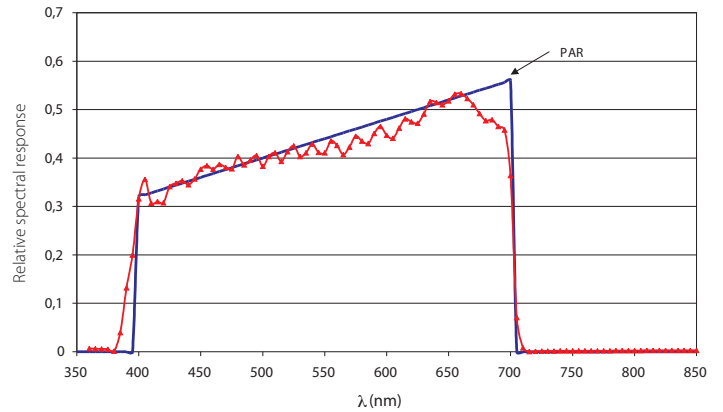


LP471RAD - Probe for the measure of IRRADIANCE				
Measuring range (W/m ²):	1.0·10 ⁻³ ...999.9·10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1·10 ⁻³	0.001	0.01	0.1
Spectral range:	400nm...1050nm			
Calibration uncertainty:	<5%			
f ₂ (response according to the cosine law):	<6%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	±1 digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<1%			
Working temperature:	0...50°C			

Radiometric probe for **IRRADIANCE** measurement in the spectral range 400 nm...1050 nm, diffuser for cosine correction. Measurement range: 1.0·10⁻³ W/m²...2000 W/m².



Typical response curve: LP471RAD

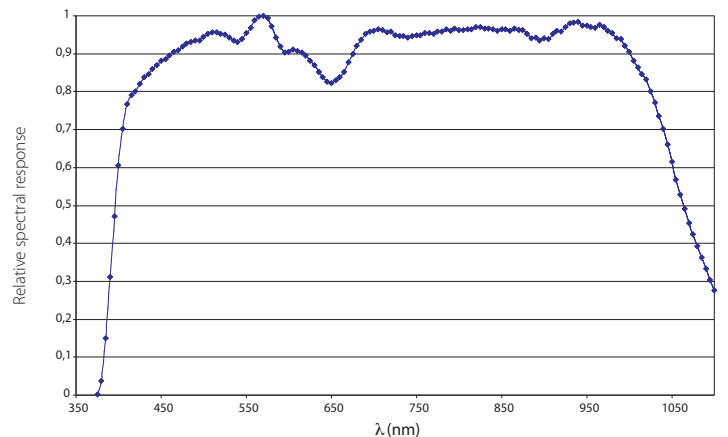


LP471UVA - Probe for the measure of UVA IRRADIANCE				
Measuring range (W/m ²):	1.0 · 10 ⁻³ ...999.9 · 10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1 · 10 ⁻³	0.001	0.01	0.1
Spectral range:	315 nm...400 nm (Peak 360nm)			
Calibration uncertainty:	<5%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	±1digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

Radiometric probe for **IRRADIANCE** measurement, in the **UVA** spectral range 315 nm...400 nm, peak 360 nm.
Measurement range: 1.0 · 10⁻³ W/m² ... 2000 W/m².



Typical response curve: LP471UVA

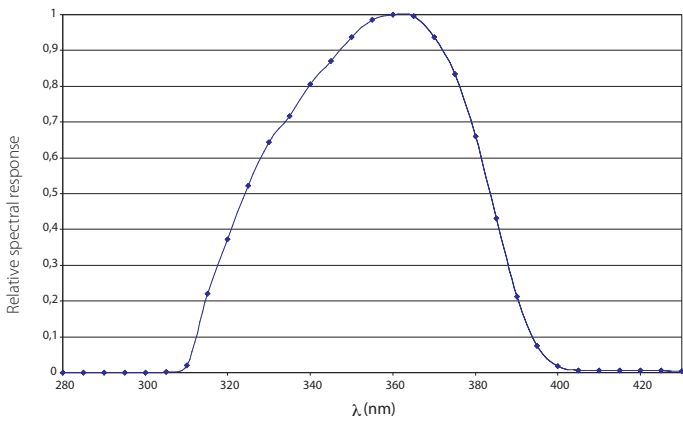


LP471UVB - Probe for the measure of UVB IRRADIANCE				
Measuring range (W/m ²):	1.0 · 10 ⁻³ ...999.9 · 10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1 · 10 ⁻³	0.001	0.01	0.1
Spectral range:	280nm...315nm (Peak 305nm...310nm)			
Calibration uncertainty:	<5%			
f ₃ (linearity):	<2%			
f ₄ (instrument reading error):	±1digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

Radiometric probe for **IRRADIANCE** measurement in the **UVB** spectral range 280 nm...315 nm, peak 305 nm...310 nm.
Measurement range: 1.0 · 10⁻³ W/m² ... 2000 W/m².



Typical response curve: LP471UVB

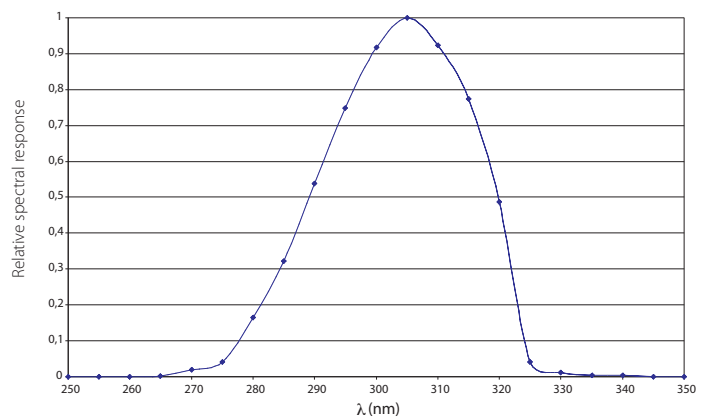


LP471UVC - Probe for the measure of UVC IRRADIANCE				
Measuring range (W/m ²):	1.0 · 10 ⁻³ ...999.9 · 10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1 · 10 ⁻³	0.001	0.01	0.1
Spectral range:	220nm...280nm (Peak 260nm)			
Calibration uncertainty:	<5%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	±1digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

Radiometric probe for **IRRADIANCE** measurement, in the **UVC** spectral range 220 nm...280 nm, peak 260 nm.
Measurement range: 1.0 · 10⁻³ W/m² ... 2000 W/m².



Typical response curve: LP471UVC

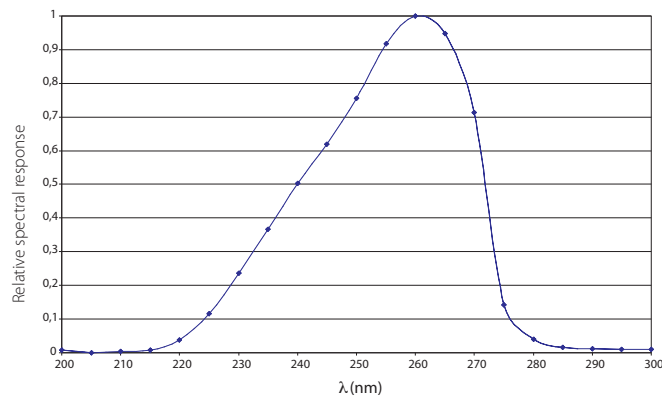


LP471UVBC - Probe for the measure of UV-BC IRRADIANCE				
Measuring range (W/m ²):	1.0 · 10 ⁻³ ...999.9 · 10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1 · 10 ⁻³	0.001	0.01	0.1
Spectral range:	210 nm...335 nm (Peak 265 nm)			
Calibration uncertainty:	<7% (calibration @ 254 nm)			
f ₃ (linearity):	<2%			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

Radiometric probe for measuring the **IRRADIANCE** in the **UV-BC** spectral range 210 nm...335 nm, peak at 265 nm.
Measurement range: 1.0 · 10⁻³ W/m² ... 2000 W/m².




Typical response curve: LP471UVBC

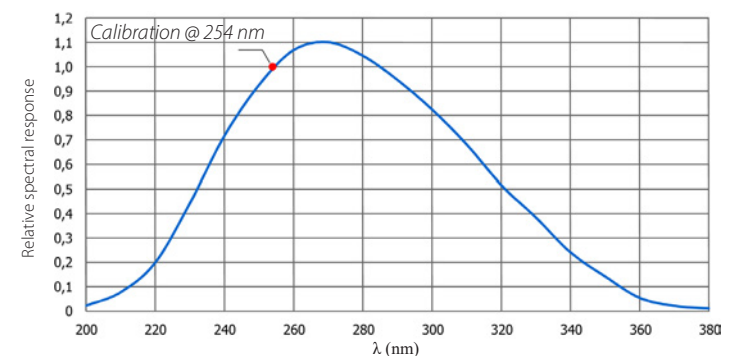


LP471BLUE - Probe for the measure of IRRADIANCE in spectral band of BLUE LIGHT				
Measurement range (W/m ²):	1.0·10 ⁻³ ... 999.9·10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1·10 ⁻³	0.001	0.01	0.01
Spectral range:	380 nm ... 550 nm. Action curve for damages of Blue light B(λ)			
Calibration uncertainty:	<10%			
f ₂ (response according to the cosine law):	<6%			
f ₃ (linearity):	<3%			
f ₄ (instrument reading error):	±1 digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

Relative spectral response

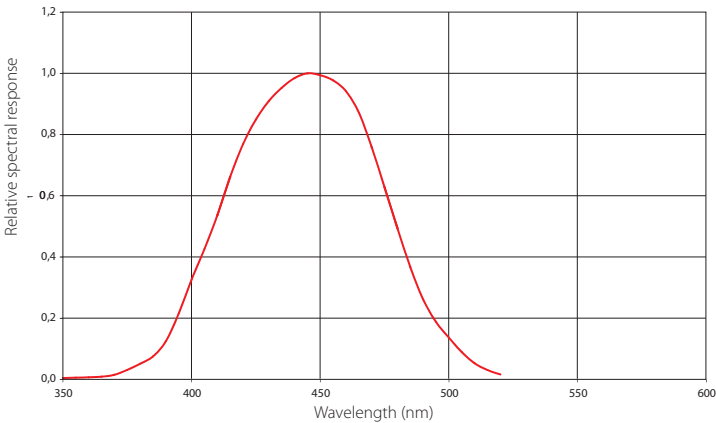

The radiometric probe **LP471BLUE** measures irradiance (W/m²) in spectral band of blue light. The probe consists of a photodiode plus an appropriate filter and it is provided with diffuser for proper measure in accordance with the cosine law. The spectral response curve of the probe allows to measure the radiation effective for damages caused by blue light (curve B(λ) according to the standards ACGIH / ICNIRP) in the spectral range from 380 nm to 550 nm. The radiation optics in this portion of the spectrum can produce photochemical damage to the retina. Another field of application is the monitoring of the probe irradiance from blue light used in the treatment of neonatal jaundice.

LP471SILICON-PYRA - Probe for the measure of GLOBAL SOLAR RADIATION				
Measurement range (W/m ²):	1.0·10 ⁻³ ... 999.9·10 ⁻³	1.000...19.999	20.00...199.99	200.0...1999.9
Resolution (W/m ²):	0.1·10 ⁻³	0.001	0.01	0.1
Spectral range:	400 nm ... 1100 nm			
Calibration uncertainty:	<3%			
f ₂ (response according to the cosine law):	<3%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	±1 digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

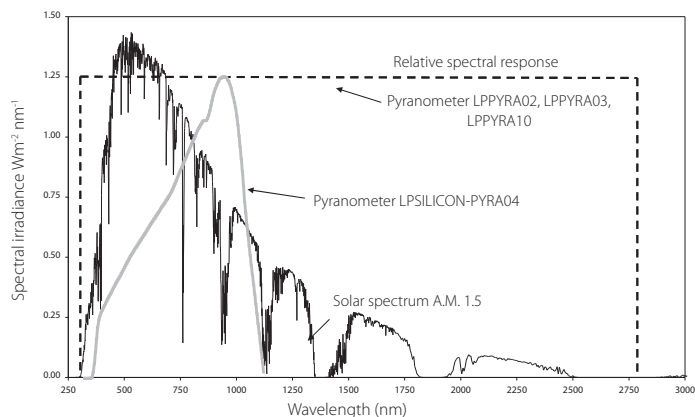


LP471P-A - Combined probe with two sensors for the measure of ILLUMINANCE and UVA IRRADIANCE				
Illuminance				
Measuring range (lux):	0.3...199.9	...1999.9	...19999	...199.99·10 ³
Resolution (lux):	0.01	0.1	1	0.01·10 ³
Spectral range:	in agreement with standard photopic curve V(λ)			
α (temp. coefficient) f ₆ (T)	<0.05%/K			
Calibration uncertainty:	<4%			
f ₁ (in agreement with photopic response V(λ)):	<6%			
f ₂ (response according to the cosine law):	<3%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	<0.5%			
f ₅ (fatigue):	<0.5%			
Class:	B			
Drift after 1 year:	<1%			
Working temperature:	0...50°C			
Reference Standards:	CIE n.69 - UNI 11142			

Please refer to the spectral response of the LP471PHOT probe.

UVA Irradiance				
Measuring range (μW/cm ²):	0.10...199.99	...1999.9	...19999	...199.99·10 ³
Resolution (μW/cm ²):	0.01	0.1	1	0.01·10 ³
Spectral range:	315 nm...400 nm (Peak 360 nm)			
Calibration uncertainty:	<5%			
f ₂ (response according to the cosine law):	<6%			
f ₃ (linearity):	<1%			
f ₄ (instrument reading error):	±1 digit			
f ₅ (fatigue):	<0.5%			
Drift after 1 year:	<2%			
Working temperature:	0...50°C			

Please refer to the spectral response of the LP471UVA probe.

LP471A-Uveff - Probe for the measure of TOTAL EFFECTIVE IRRADIANCE weighted according to the UV action curve (CEI EN 60335-2-27)	
Total Effective Irradiance	
Measuring range (W/m ²):	0.010 ... 19.999
Resolution (W/m ²):	0.001
Spectral range:	UV action curve for measuring erythema (250 nm...400 nm)
Calibration uncertainty:	<15%
f ₃ (linearity):	<3%
f ₄ (instrument reading error):	±1 digit
f ₅ (fatigue):	<0.5%
Drift after 1 year:	<2%
Working temperature:	0...50°C
UV Irradiance	
Measuring range (W/m ²):	0.1 ... 1999.9
Resolution (W/m ²):	0.1
Spectral range:	315 nm ... 400 nm
UV_BC Irradiance	
Measuring range (W/m ²):	0.010 ... 19.999
Resolution (W/m ²):	0.001
Spectral range:	250 nm ... 315 nm

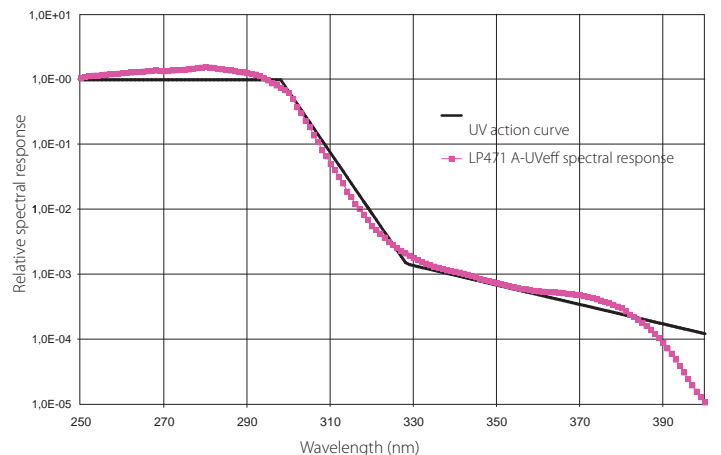

Архангельск (8182)63-90-72	Ижевск (3412)26-03-58	Магнитогорск (3519)55-03-13	Пермь (342)205-81-47	Сургут (3462)77-98-35
Астана (7172)727-132	Иркутск (395)279-98-46	Москва (495)268-04-70	Ростов-на-Дону (863)308-18-15	Тверь (4822)63-31-35
Астрахань (8512)99-46-04	Казань (843)206-01-48	Мурманск (8152)59-64-93	Рязань (4912)46-61-64	Томск (3822)98-41-53
Барнаул (3852)73-04-60	Калининград (4012)72-03-81	Набережные Челны (8552)20-53-41	Самара (846)206-03-16	Тула (4872)74-02-29
Белгород (4722)40-23-64	Калуга (4842)92-23-67	Нижний Новгород (831)429-08-12	Санкт-Петербург (812)309-46-40	Тюмень (3452)66-21-18
Брянск (4832)59-03-52	Кемерово (3842)65-04-62	Новокузнецк (3843)20-46-81	Саратов (845)249-38-78	Ульяновск (8422)24-23-59
Владивосток (423)249-28-31	Киров (8332)68-02-04	Новосибирск (383)227-86-73	Севастополь (8692)22-31-93	Уфа (347)229-48-12
Волгоград (844)278-03-48	Краснодар (861)203-40-90	Омск (3812)21-46-40	Симферополь (3652)67-13-56	Хабаровск (4212)92-98-04
Вологда (8172)26-41-59	Красноярск (391)204-63-61	Орел (4862)44-53-42	Смоленск (4812)29-41-54	Челябинск (351)202-03-61
Воронеж (473)204-51-73	Курск (4712)77-13-04	Оренбург (3532)37-68-04	Сочи (862)225-72-31	Череповец (8202)49-02-64
Екатеринбург (343)384-55-89	Липецк (4742)52-20-81	Пенза (8412)22-31-16	Ставрополь (8652)20-65-13	Ярославль (4852)69-52-93
Иваново (4932)77-34-06	Киргизия (996)312-96-26-47	Казахстан (772)734-952-31	Таджикистан (992)427-82-92-69	

Единый адрес для всех регионов: dmh@nt-rt.ru || www.deltaohm.nt-rt.ru